

# Medical Spectrum

## Overview

This guide provides instruction on configuring both Medical-Objects Download Client (Capricorn) and Medical Spectrum software to import electronic results.

If you require any assistance with the installation or configuration, or if you have any questions, please contact the Medical-Objects Helpdesk on (07) 5456 6000.

If you have not Installed the Medical-Objects Download client, Please see the guide for [Installing Capricorn on Windows](#).

## Configuring Capricorn Software

### Accessing the Capricorn Configuration Window

Note:

In some cases, the Capricorn may be configured as a service. See [this guide](#) for instructions on how to launch the Capricorn if it is set up as a service.

1. To launch the HL7 Tray application, Go to **Start Menu, All Programs, Medical-Objects** and select the **Medical-Objects Capricorn**. Alternatively, You can go to **C:\MO\Capricorn** and run the **Capricorn.exe**.
2. The following icon will appear in the tray. Double click on it to bring up the log window.




3. When the log window is displayed, Click on the **Configuration** icon highlighted below, or select **Utility** and select **Configuration**.



### Capricorn Configuration Settings

1. Click on **Ack Management**.

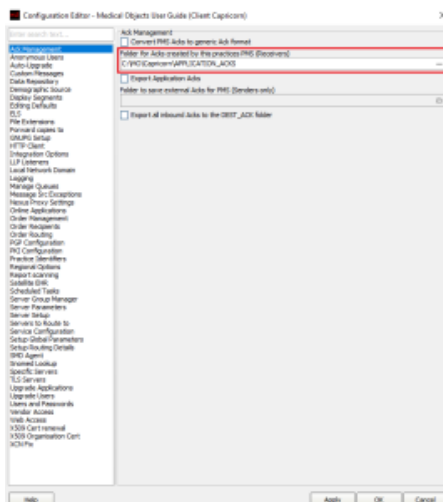


- 1 Overview
- 2 Configuring Capricorn Software
  - 2.1 Accessing the Capricorn Configuration Window
  - 2.2 Capricorn Configuration Settings
- 3 Configuring Medical Spectrum Classic
  - 3.1 Medical-Objects Letters
  - 3.2 Medical-Objects Pathology
  - 3.3 Medical-Objects Radiology
- 4 Importing a Result into Medical Spectrum

- Set the **ACKManagement** Path to the following path:

C:\MO\Capricorn\APPLICATION\_ACKS

- Select the **Integration Options** in the left panel.
- Make sure at the bottom of the panel that under **Incoming Modifier** that **Spectrum HL7 Modifier** is set, as shown below.

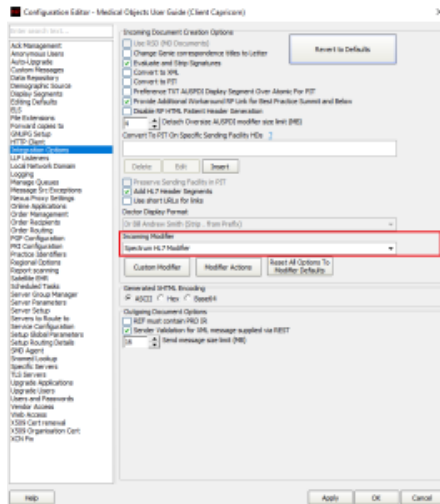


Important:



Older versions of Spectrum will **NOT** import **ORU** or **HL7** files that have file names over 9 Characters long. It does not have this problem with PIT files, so be sure to convert the files to PIT. The 9 Character limit also affects file paths. so if your results are in a folder called **INCOMIN G RESULTS** for example. It will not look in that path.

- In the left hand side panel, select **Server Parameters**.
- In **Message Output Directory (Main)**, Enter the path for letters to be imported in to. For example:

C:\MO\Letters\

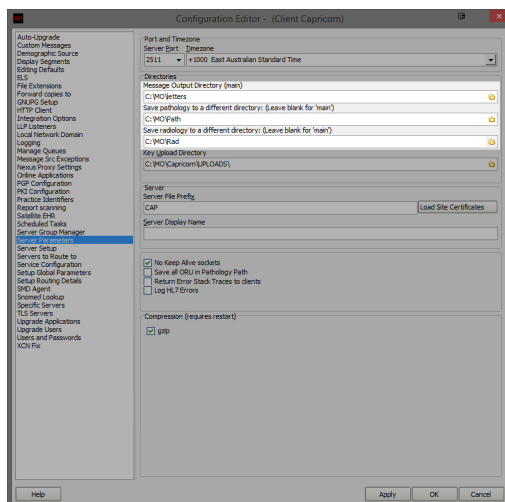

- Enter the Pathology and Radiology paths as shown above.

```
Pathology - C:\MO\Path  
Radiology - C:\MO\Rad
```

8. Click **Apply** and **OK**.

The Configuration for Medical Spectrum is complete.


## Configuring Medical Spectrum Classic

### Medical-Objects Letters


1. Open Medical Spectrum.



2. Click on the **System** icon.
3. The following window will open.

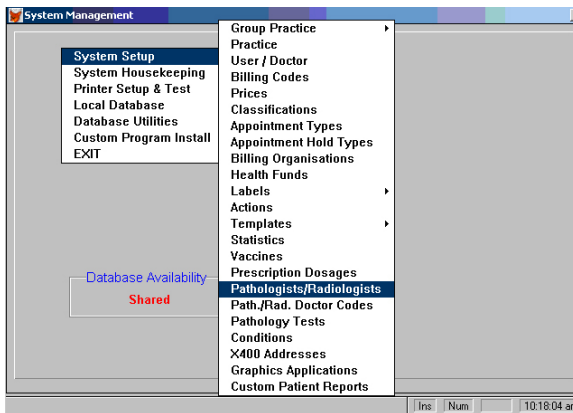

4. Click **System Setup**.
5. Click **Pathologists/Radiologists**.

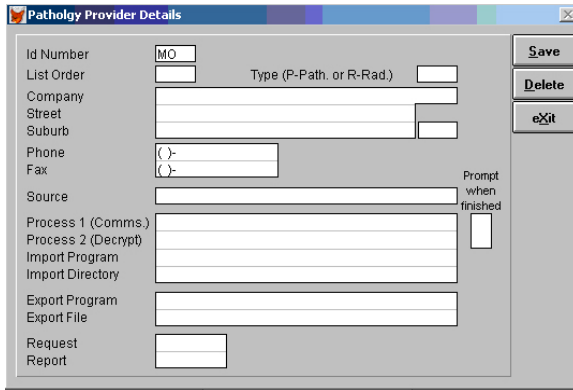


The 'Pathology Provider Details' dialog box contains the following fields and controls:


- Id Number:** Text field containing 'MO'.
- List Order:** Text field.
- Type (P-Path. or R-Rad.):** Text field.
- Company:** Text field.
- Street:** Text field.
- Suburb:** Text field.
- Phone:** Text field with a '( )-' prefix.
- Fax:** Text field with a '( )-' prefix.
- Source:** Text field.
- Process 1 (Comms.):** Text field.
- Process 2 (Decrypt):** Text field.
- Import Program:** Text field.
- Import Directory:** Text field.
- Export Program:** Text field.
- Export File:** Text field.
- Request Report:** Text field.
- Buttons:** 'Save', 'Delete', and 'eXit' buttons are located on the right side.
- Prompt when finished:** A checkbox.

6. Enter MO in the **Id Number** field and press TAB.

Note:

 Make sure you backspace to the left in the ID Number field to avoid blanks; you cannot delete an entry once it has been created. If MO is already configured, press TAB to call up the details. You can also select Medical-Objects from the available drop down list; this will display the ID Number only. Press TAB to call up the details.


7. If it is a new record, the following window will appear.

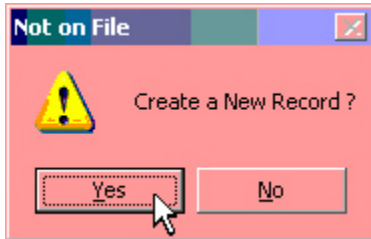

The 'Not on File' dialog box contains the following elements:

- Title Bar:** 'Not on File'.
- Icon:** A yellow warning triangle with an exclamation mark.
- Text:** 'Create a New Record ?'.
- Buttons:** 'Yes' and 'No' buttons.

8. Click **Yes**.

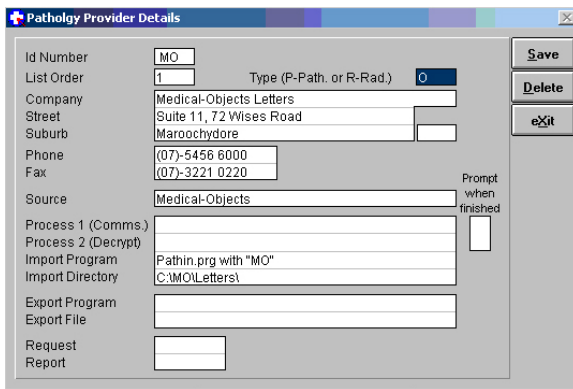


The 'Pathology Provider Details' dialog box is now populated with the following data:

- Id Number:** MO
- List Order:** 1
- Type (P-Path. or R-Rad.):** 0
- Company:** Medical-Objects Letters
- Street:** Suite 11, 72 Wises Road
- Suburb:** Maroochydore
- Phone:** (07)-5456 6000
- Fax:** (07)-3221 0220
- Source:** Medical-Objects
- Process 1 (Comms.):**
- Process 2 (Decrypt):**
- Import Program:** Pathin.prg with "MO"
- Import Directory:** C:\MO\Letters\
- Export Program:**
- Export File:**
- Request Report:**

9. Enter in the above information (Make sure your data is accurate as you cannot delete the contact once it has been saved).
10. Click **Save**.
11. Click **Exit**.

## Medical-Objects Pathology


1. We follow the same steps taken in the first section as shown below.

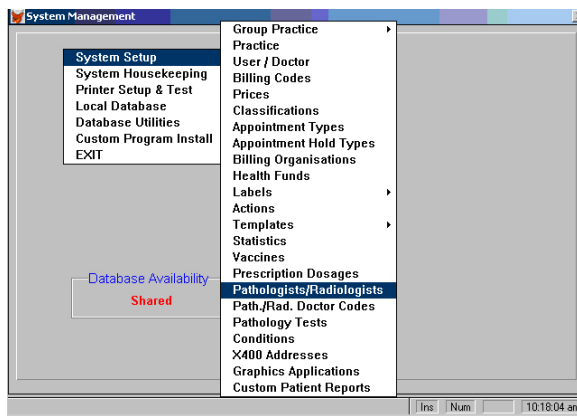

2. Enter MP in the **Id Number** field and press TAB.

The screenshot shows the 'Pathology Provider Details' window. The 'Id Number' field contains the text 'MP'. Other fields include 'List Order', 'Type (P-Path. or R-Rad.)', 'Company', 'Street', 'Suburb', 'Phone', 'Fax', 'Source', 'Process 1 (Comms.)', 'Process 2 (Decrypt)', 'Import Program', 'Import Directory', 'Export Program', 'Export File', 'Request', and 'Report'. There are buttons for 'Save', 'Delete', and 'Exit' on the right side. A 'Prompt when finished' checkbox is also present.

3. If it is a new record the following window will appear.

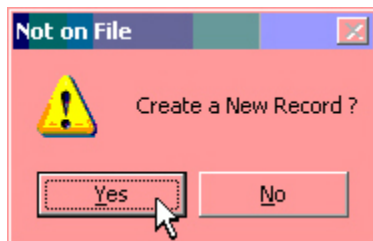


4. Click **Yes**.

The screenshot shows the 'Pathology Provider Details' window after the 'Yes' button was clicked. The 'Id Number' field is 'MP'. The 'List Order' field is '1'. The 'Type (P-Path. or R-Rad.)' field is 'P'. The 'Company' field is 'Medical-Objects Pathology'. The 'Street' field is 'Suite 11, 72 Wises Road'. The 'Suburb' field is 'Maroochydore' and the 'Postcode' field is '4558'. The 'Phone' field is '(07)-5456 6000' and the 'Fax' field is '(07)-3221 0220'. The 'Source' field is 'Medical-Objects'. The 'Import Program' field is 'Pathin.prg with "MP"' and the 'Import Directory' field is 'C:\MO\Path\'. The 'Export Program' and 'Export File' fields are empty. The 'Request' and 'Report' fields are also empty. The 'Save', 'Delete', and 'Exit' buttons are on the right. The 'Prompt when finished' checkbox is checked.

5. Enter in the above information (Make sure your data is accurate as you cannot delete the contact once it has been saved)
6. Click **Save**.
7. Click **Exit**.

## Medical-Objects Radiology


1. We follow the same steps taken in the first and second sections as shown below.

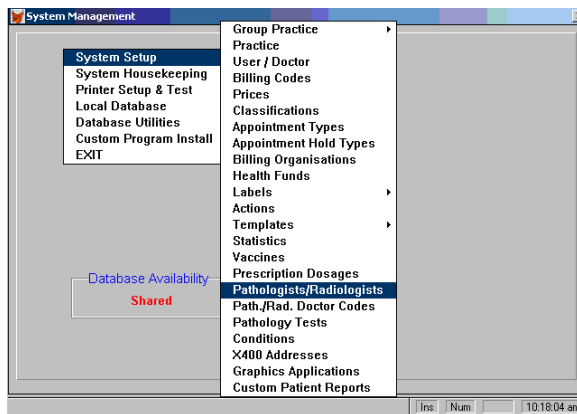

2. Enter **MR** in the **Id Number** and press TAB.

The screenshot shows the 'Pathology Provider Details' window. The 'Id Number' field contains 'MR'. The 'List Order' field is empty. The 'Type (P-Path. or R-Rad.)' field is empty. The 'Company' field is empty. The 'Street' field is empty. The 'Suburb' field is empty. The 'Phone' field is empty. The 'Fax' field is empty. The 'Source' field is empty. The 'Process 1 (Comms.)' field is empty. The 'Process 2 (Decrypt)' field is empty. The 'Import Program' field is empty. The 'Import Directory' field is empty. The 'Export Program' field is empty. The 'Export File' field is empty. The 'Request Report' field is empty. The 'Save', 'Delete', and 'Exit' buttons are visible on the right.

3. If it is a new record the following window will appear.

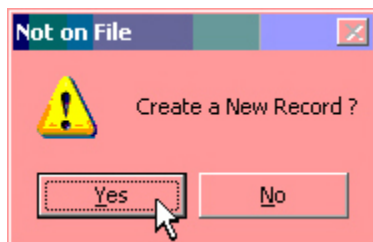

4. Click **Yes**.

The screenshot shows the 'Pathology Provider Details' window after clicking 'Yes'. The 'Id Number' field contains 'MR'. The 'List Order' field contains '1'. The 'Type (P-Path. or R-Rad.)' field contains 'R'. The 'Company' field contains 'Medical-Objects Radiology'. The 'Street' field contains 'Suite 11, 72 Wises Road'. The 'Suburb' field contains 'Maroochydore' and the 'Postcode' field contains '4558'. The 'Phone' field contains '(07)-5456 6000'. The 'Fax' field contains '(07)-3221 0220'. The 'Source' field contains 'Medical-Objects'. The 'Process 1 (Comms.)' field is empty. The 'Process 2 (Decrypt)' field is empty. The 'Import Program' field contains 'Pathin.prg with "MR"'. The 'Import Directory' field contains 'C:\MO\Rad\'. The 'Export Program' field is empty. The 'Export File' field is empty. The 'Request Report' field is empty. The 'Save', 'Delete', and 'Exit' buttons are visible on the right.


5. Enter in the above information (Make sure your data is accurate as you cannot delete the contact once it has been saved).
6. Click **Save**.
7. Click **Exit**.

## Importing a Result into Medical Spectrum


1. Click the **Medical** Icon.



2. Click the **Communication** drop-down list.

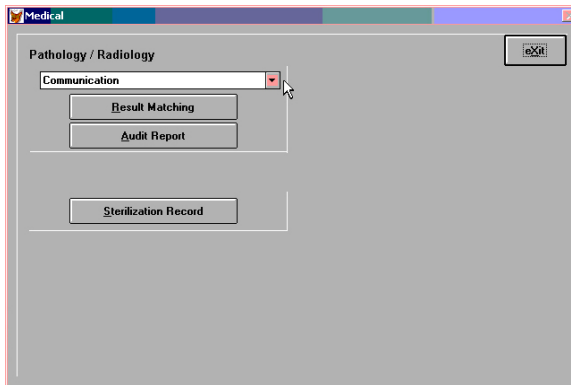


3. Select **Medical-Objects Letters**, **Medical-Objects Pathology**, or **Medical-Objects Radiology** to see what results have arrived.

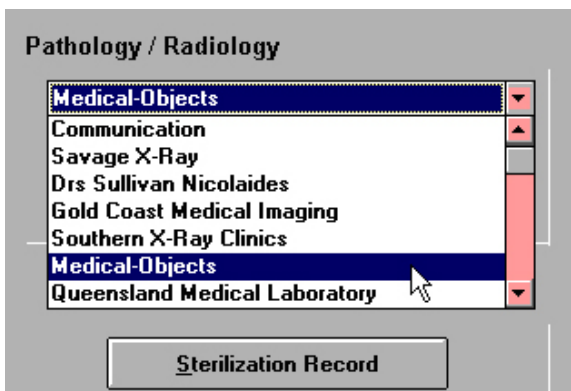


Note:



If there are any results, the number of results imported will show. If there are no results, this number will be 0.

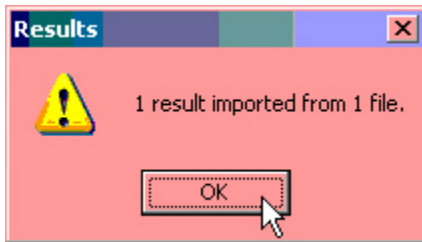


4. Click **OK**.

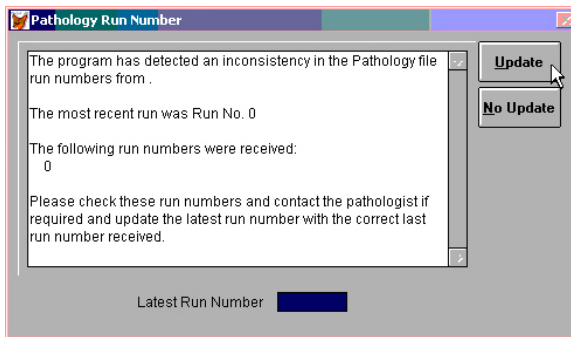


5. Click the **Update** at the **Pathology Run Number** message.




6. Click **Result Matching** to see if any results require matching.
7. The following window is displayed.

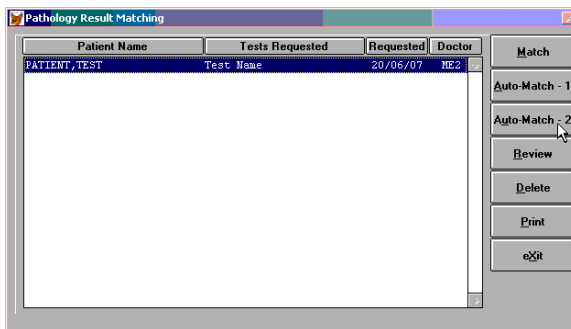

8. Click **Auto-Match -2**.

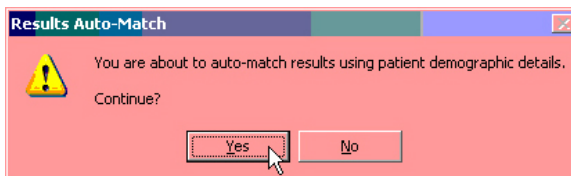

9. Click **Yes**.

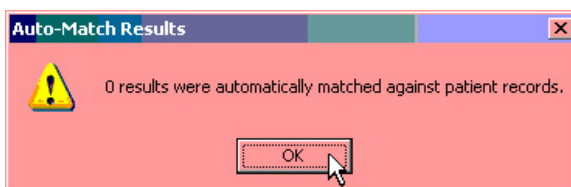



10. Click **OK**.

11. Click **Exit** on the **Pathology Result Matching** window.

12. Click **Exit** on the **Medical** window.

Note:



You should now be back to the main window.