

Medical Spectrum

Overview

This guide provides instruction on configuring both Medical-Objects Download Client (Capricorn) and Medical Spectrum software to import electronic results.

If you require any assistance with the installation or configuration, or if you have any questions, please contact the Medical-Objects Helpdesk on (07) 5456 6000.

If you have not Installed the Medical-Objects Download client, Please see the guide for [Installing Capricorn on Windows](#).

Configuring Capricorn Software

Accessing the Capricorn Configuration Window

Note:

In some cases, the Capricorn may be configured as a service. See [this guide](#) for instructions on how to launch the Capricorn if it is set up as a service.

1. To launch the HL7 Tray application, Go to **Start Menu, All Programs, Medical-Objects** and select the **Medical-Objects Capricorn**. Alternatively, You can go to **C:\MO\Capricorn** and run the **Capricorn.exe**.
2. The following icon will appear in the tray. Double click on it to bring up the log window.




3. When the log window is displayed, Click on the **Configuration** icon highlighted below, or select **Utility** and select **Configuration**.



Capricorn Configuration Settings

1. Click on **Ack Management**.

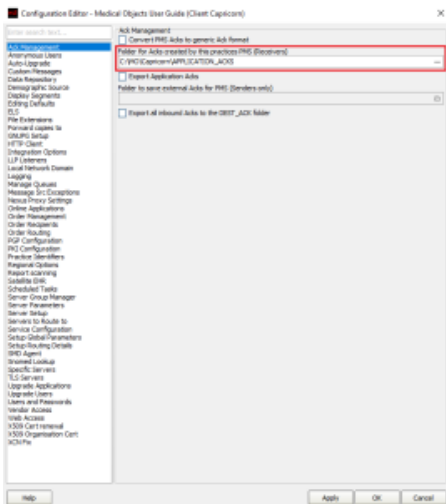


- 1 Overview
- 2 Configuring Capricorn Software
 - 2.1 Accessing the Capricorn Configuration Window
 - 2.2 Capricorn Configuration Settings
- 3 Configuring Medical Spectrum Classic
 - 3.1 Medical-Objects Letters
 - 3.2 Medical-Objects Pathology
 - 3.3 Medical-Objects Radiology
- 4 Importing a Result into Medical Spectrum

- Set the **ACKManagement** Path to the following path:

C:\MO\Capricorn\APPLICATION_ACKS

- Select the **Integration Options** in the left panel.
- Make sure at the bottom of the panel that under **Incoming Modifier** that **Spectrum HL7 Modifier** is set, as shown below.

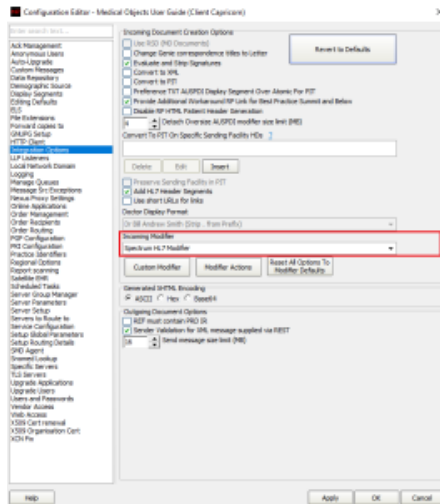


Important:



Older versions of Spectrum will **NOT** import **ORU** or **HL7** files that have file names over 9 Characters long. It does not have this problem with PIT files, so be sure to convert the files to PIT. The 9 Character limit also affects file paths. so if your results are in a folder called **INCOMIN G RESULTS** for example. It will not look in that path.

- In the left hand side panel, select **Server Parameters**.
- In **Message Output Directory (Main)**, Enter the path for letters to be imported in to. For example:

C:\MO\Letters\

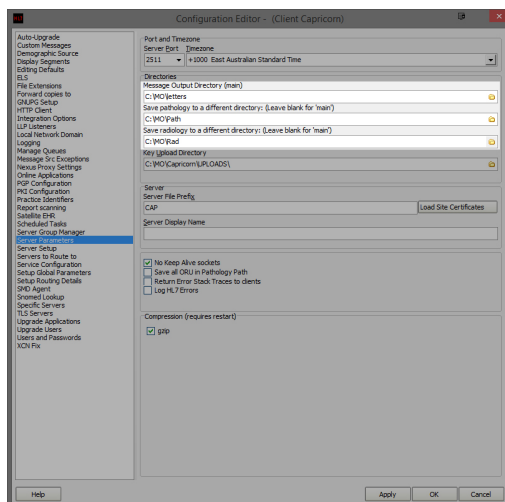

- Enter the Pathology and Radiology paths as shown above.

```
Pathology - C:\MO\Path  
Radiology - C:\MO\Rad
```

8. Click **Apply** and **OK**.

The Configuration for Medical Spectrum is complete.


Configuring Medical Spectrum Classic

Medical-Objects Letters


1. Open Medical Spectrum.



2. Click on the **System** icon.
3. The following window will open.

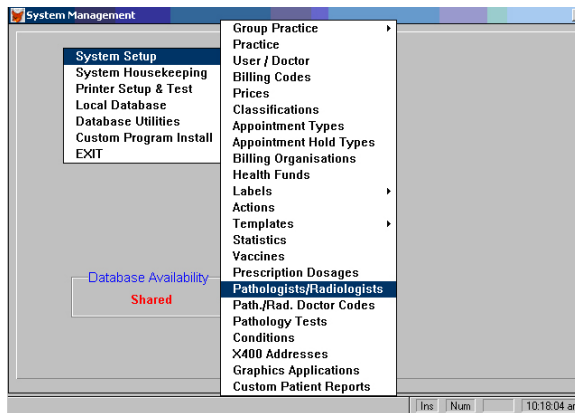

4. Click **System Setup**.
5. Click **Pathologists/Radiologists**.

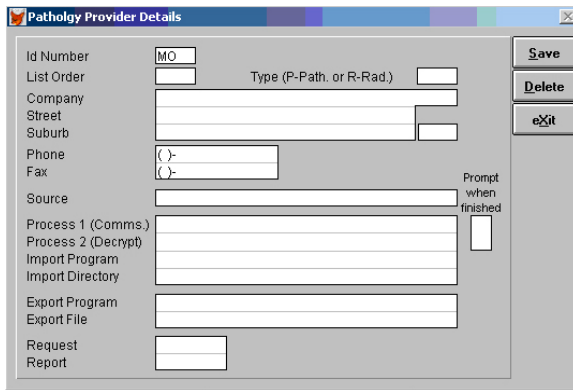


The dialog box 'Pathology Provider Details' contains the following fields:

- Id Number: MO
- List Order: (empty)
- Type (P-Path. or R-Rad.): (empty)
- Company: (empty)
- Street: (empty)
- Suburb: (empty)
- Phone: ()-()-()-()-()-()
- Fax: ()-()-()-()-()-()
- Source: (empty)
- Process 1 (Comms.): (empty)
- Process 2 (Decrypt): (empty)
- Import Program: (empty)
- Import Directory: (empty)
- Export Program: (empty)
- Export File: (empty)
- Request Report: (empty)


Buttons: Save, Delete, eXit. A checkbox 'Prompt when finished' is also present.

- Enter MO in the **Id Number** field and press TAB.

Note:


 Make sure you backspace to the left in the ID Number field to avoid blanks; you cannot delete an entry once it has been created. If MO is already configured, press TAB to call up the details. You can also select Medical-Objects from the available drop down list; this will display the ID Number only. Press TAB to call up the details.

- If it is a new record, the following window will appear.

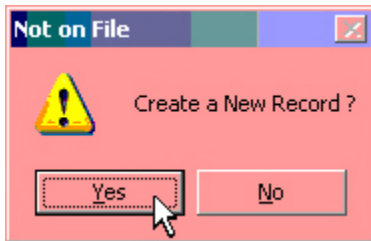

The dialog box 'Not on File' contains a yellow warning triangle icon and the text 'Create a New Record ?'. It has two buttons: Yes and No. A mouse cursor is pointing at the Yes button.

- Click **Yes**.

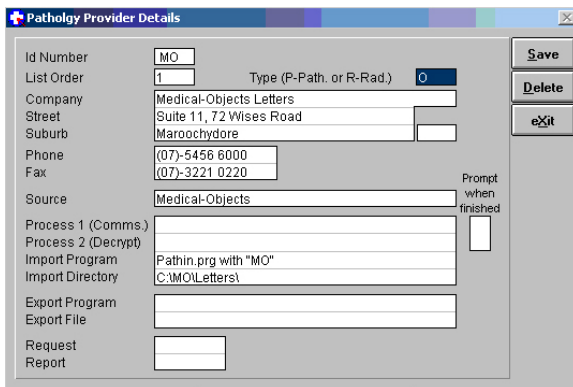

The dialog box 'Pathology Provider Details' is now populated with the following data:


- Id Number: MO
- List Order: 1
- Type (P-Path. or R-Rad.): 0
- Company: Medical-Objects Letters
- Street: Suite 11, 72 Wises Road
- Suburb: Maroochydore
- Phone: (07)-5456 6000
- Fax: (07)-3221 0220
- Source: Medical-Objects
- Process 1 (Comms.): (empty)
- Process 2 (Decrypt): (empty)
- Import Program: Pathin.prg with "MO"
- Import Directory: C:\MO\Letters\
- Export Program: (empty)
- Export File: (empty)
- Request Report: (empty)

Buttons: Save, Delete, eXit. A checkbox 'Prompt when finished' is also present.

- Enter in the above information (Make sure your data is accurate as you cannot delete the contact once it has been saved).
- Click **Save**.
- Click **Exit**.

Medical-Objects Pathology


- We follow the same steps taken in the first section as shown below.

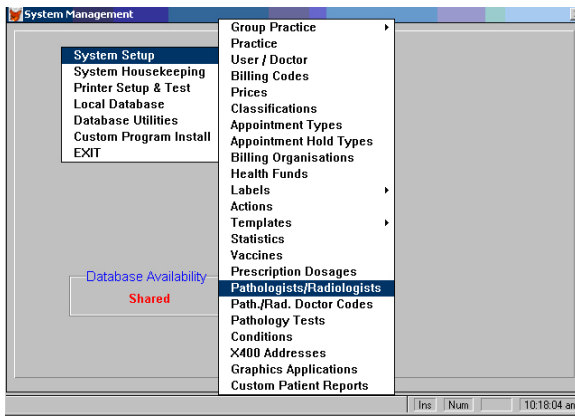

2. Enter MP in the **Id Number** field and press TAB.

The screenshot shows the 'Pathology Provider Details' window. The 'Id Number' field contains 'MP'. Other fields include 'List Order', 'Type (P-Path. or R-Rad.)', 'Company', 'Street', 'Suburb', 'Phone', 'Fax', 'Source', 'Process 1 (Comms.)', 'Process 2 (Decrypt)', 'Import Program', 'Import Directory', 'Export Program', 'Export File', 'Request', and 'Report'. There are 'Save', 'Delete', and 'Exit' buttons on the right. A 'Prompt when finished' checkbox is also present.

3. If it is a new record the following window will appear.

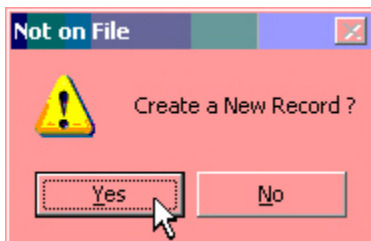


4. Click **Yes**.

The screenshot shows the 'Pathology Provider Details' window after clicking 'Yes'. The fields are now populated: 'Id Number' is 'MP', 'List Order' is '1', 'Type (P-Path. or R-Rad.)' is 'P', 'Company' is 'Medical-Objects Pathology', 'Street' is 'Suite 11, 72 Wises Road', 'Suburb' is 'Maroochydore' with postcode '4558', 'Phone' is '(07)-5456 6000', 'Fax' is '(07)-3221 0220', 'Source' is 'Medical-Objects', 'Import Program' is 'Pathin.prg with "MP"', and 'Import Directory' is 'C:\MO\Path\'. The 'Save', 'Delete', and 'Exit' buttons are still on the right.

5. Enter in the above information (Make sure your data is accurate as you cannot delete the contact once it has been saved)
6. Click **Save**.
7. Click **Exit**.

Medical-Objects Radiology


1. We follow the same steps taken in the first and second sections as shown below.

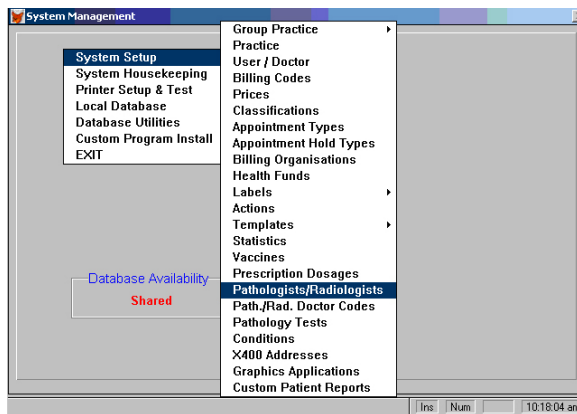

2. Enter **MR** in the **Id Number** and press TAB.

The screenshot shows the 'Pathology Provider Details' window. The 'Id Number' field is set to 'MR'. The 'List Order' field is empty. The 'Type (P-Path. or R-Rad.)' field is empty. The 'Company' field is empty. The 'Street' field is empty. The 'Suburb' field is empty. The 'Phone' field is empty. The 'Fax' field is empty. The 'Source' field is empty. The 'Process 1 (Comms.)' field is empty. The 'Process 2 (Decrypt)' field is empty. The 'Import Program' field is empty. The 'Import Directory' field is empty. The 'Export Program' field is empty. The 'Export File' field is empty. The 'Request Report' field is empty. The 'Save', 'Delete', and 'Exit' buttons are visible on the right.

3. If it is a new record the following window will appear.

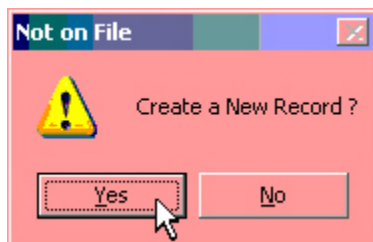

4. Click **Yes**.

The screenshot shows the 'Pathology Provider Details' window. The 'Id Number' field is set to 'MR'. The 'List Order' field is set to '1'. The 'Type (P-Path. or R-Rad.)' field is set to 'R'. The 'Company' field is set to 'Medical-Objects Radiology'. The 'Street' field is set to 'Suite 11, 72 Wisers Road'. The 'Suburb' field is set to 'Maroccydore'. The 'Phone' field is set to '(07)-5456 6000'. The 'Fax' field is set to '(07)-3221 0220'. The 'Source' field is set to 'Medical-Objects'. The 'Process 1 (Comms.)' field is empty. The 'Process 2 (Decrypt)' field is empty. The 'Import Program' field is set to 'Pathin.prg with "MR"'. The 'Import Directory' field is set to 'C:\MO\Rad\'. The 'Export Program' field is empty. The 'Export File' field is empty. The 'Request Report' field is empty. The 'Save', 'Delete', and 'Exit' buttons are visible on the right.


5. Enter in the above information (Make sure your data is accurate as you cannot delete the contact once it has been saved).
6. Click **Save**.
7. Click **Exit**.

Importing a Result into Medical Spectrum


1. Click the **Medical** Icon.



2. Click the **Communication** drop-down list.

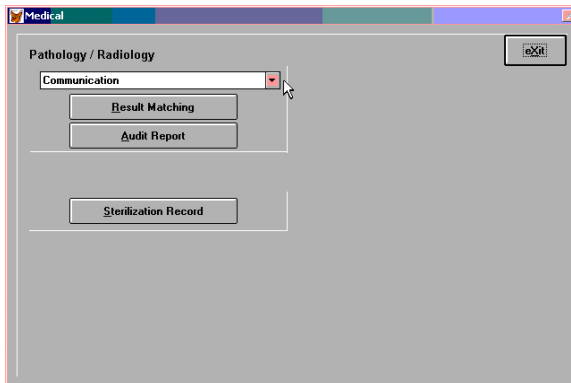


3. Select **Medical-Objects Letters**, **Medical-Objects Pathology**, or **Medical-Objects Radiology** to see what results have arrived.

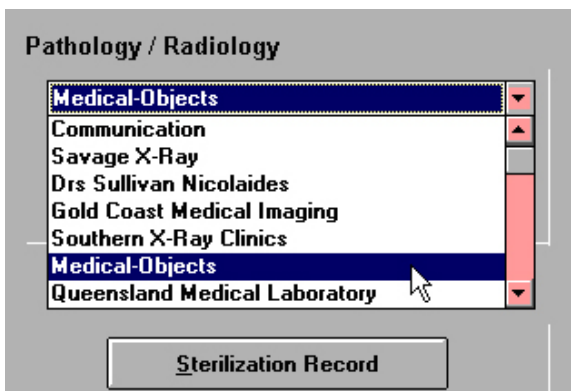


Note:



If there are any results, the number of results imported will show. If there are no results, this number will be 0.

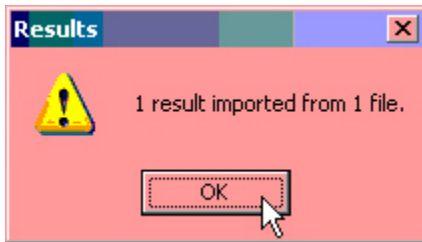


- Click **OK**.

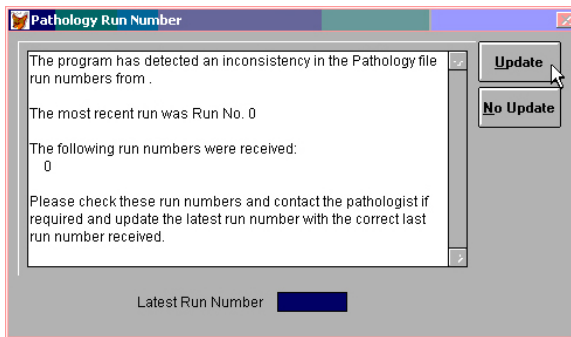


- Click the **Update** at the **Pathology Run Number** message.




- Click **Result Matching** to see if any results require matching.
- The following window is displayed.

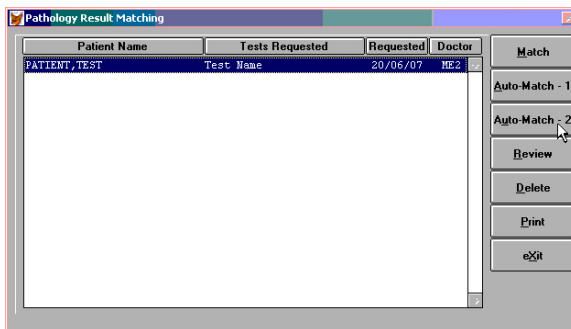

- Click **Auto-Match -2**.

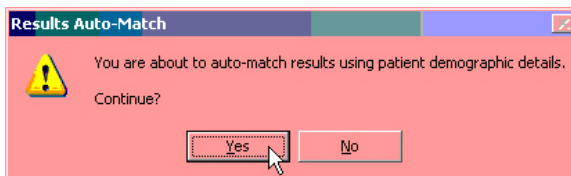

- Click **Yes**.

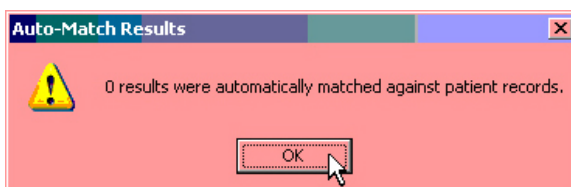

10. Click **OK**.

11. Click **Exit** on the **Pathology Result Matching** window.

12. Click **Exit** on the **Medical** window.

Note:



You should now be back to the main window.